


Monitoring Devices

Date Range 01 Oct 2023 - 31 Oct 2023


Device Serial	Monitoring Points
HEX-000390	Site Compound

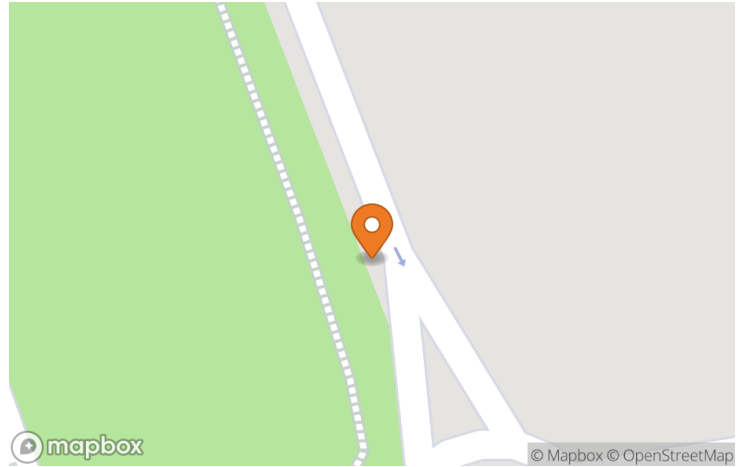

Dust Monitoring Graphs

Site Compound

01 Oct 2023 - 31 Oct 2023

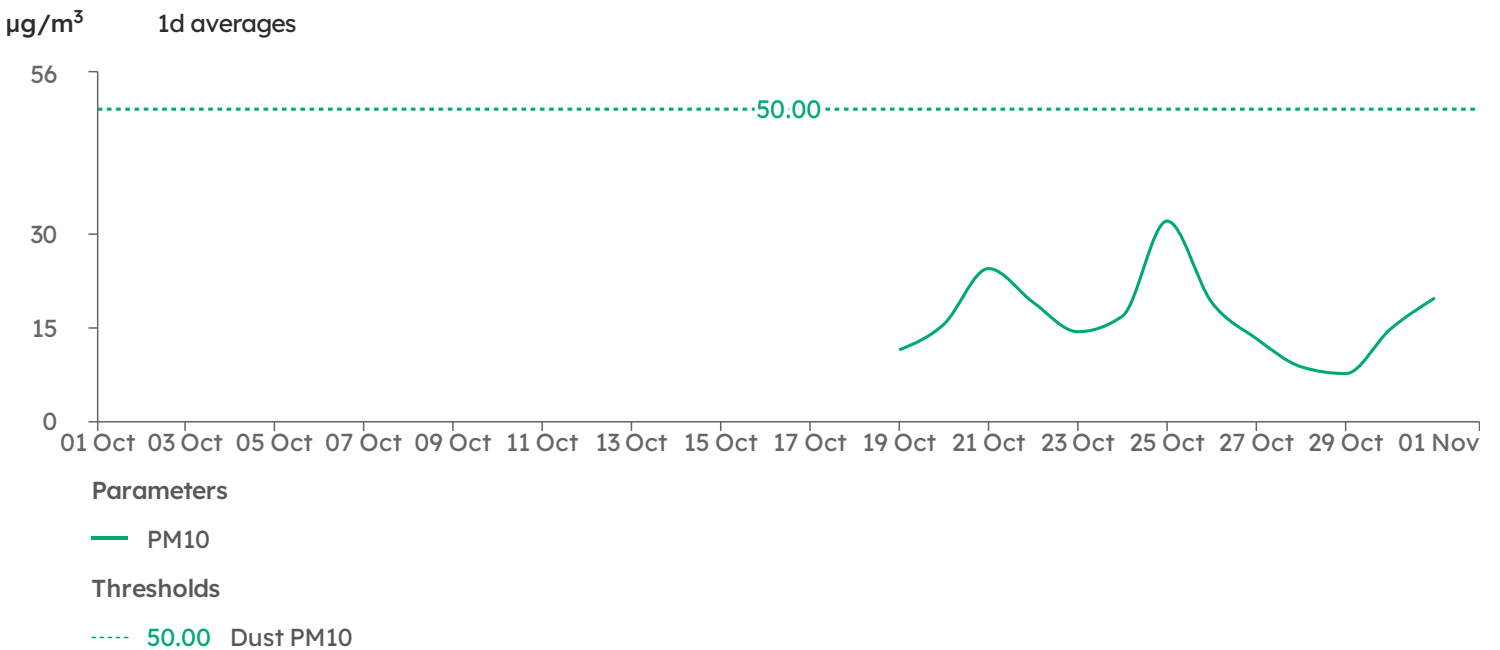

Device Details

Device Serial	Monitoring Points	Model	Calibration Date	Calibration Due
HEX-000390	Site Compound	SiteHive Hexanode	29 Aug 2023	29 Aug 2025